

HALCYON™ CHAMBIOS

Photo: Michael Westreicher



Table of Contents

Table of Contents	1
Introduction	3
1.1 Safety Considerations	3
1.2 Warnings	4
1.3 Installation	5
1.4 Operation	6
Powering On	6
Two-Button Operation	7
Custom Field	7
Custom Function	8
1.5 Surface Mode	8
1.6 Care and Maintenance	8
Charging and USB Connection	9
2 Settings	10
2.1 Menu	11
2.2 Select a Gas	15
2.3 Edit a Gas Setting from the Gas Table	16
Editing Gas Content	16
Enabling/Disabling a Gas	16
Presets	16
2.4 Pairing	17
Wireless Interface	17
Pairing a SYMBIOS Tank Pod	17
Pairing a SYMBIOS Tank Pod with Gas in the Gas Table	17
Pairing a SYMBIOS Tank Pod Independently from the Gas Table	18
Pairing the Trim Sensor	18
Calibrating the Trim Sensor	19
Pairing a SYMBIOS CM eCCR	19
2.5 Compass Calibration	20
3 Diving	20
3.1 Preparations Before the Dive	22
3.2 Decompression Model	23
3.3 Time To Surface (TTS) Calculation	23
3.4 Training Mode	24
3.5 Dive Modes	24
3.6 Open Circuit Diving	24
Diving with Air (NX21)	24
Decompression Diving	25
Safety Stop Indicator	26

Auxiliary Screen	26
Diving with NITROX	26
Diving with TRIMIX	27
Gas Switches	27
Deco Screen	27
Tissues Loading Screen	28
After the Dive	28
3.7 Closed Circuit Diving	30
Preparation	30
O2 Sensor Calibration	30
Diving	30
Bailout	31
3.8 Closed Circuit Diving with Fixed Setpoint	32
3.9 Bottom Timer	33
3.10 Sidemount Diving	34
3.11 Navigation	35
3.12 Alarms and Notifications	36
Notifications in Sidemount Mode	38
Alarms in CCR mode	38
4 Specifications	40
4.1 General Specifications	40
4.2 Decompression Algorithm	40
4.3 Electrical specifications	40
4.4 Dive data storage	41
4.5 Testing and validation	41
5 Troubleshooting	41
6 Firmware Update	42
7 Warranty	42
7.1 Limitations of Liability	43
8 CE	44
9 Identification	45
9.1 FCC	45
10 Info	46

Introduction

Thank you for purchasing the SYMBIOS HUD dive computer. The SYMBIOS HUD is an advanced dive computer built from the toughest materials on the market and highly sophisticated electronic components. The Hybrid Transflective Color Screen display is extremely easy to read, even in bright sunlight.

The SYMBIOS HUD can be used as a dive computer for air, NITROX, TRIMIX, and closed circuit rebreather diving.

The SYMBIOS HUD also features an innovative wireless interface. This interface allows data reception from multiple sources.

Currently, the device can receive wireless data from:

- SYMBIOS Tank Pod
- SYMBIOS pO₂ Transmitter
- SYMBIOS pO₂ Transmitter, P-Port version
- SYMBIOS CM eCCR
- SYMBIOS GPS Buoy
- DPV equipped with a Halcyon SYMBIOS-compatible wireless transmitter
- External compass
- SYMBIOS wireless OEM interface

The SYMBIOS HUD, together with a compatible SYMBIOS Tank Pod, is classified as Personal Protective Equipment under the EU Regulation 2016/425 and protects against risks listed under PPE Risk Category III (a): substances and mixtures which are hazardous to health.

Based on EU PPE Regulation 2016/425 Annex I, the SYMBIOS HUD protects the user/diver from the risk of drowning (Category III (i)) by displaying vital tank pressure information which allows for appropriate life-saving action.

1.1 Safety

Considerations

Before using the SYMBIOS HUD, please read this manual in its entirety. Be aware that diving has many inherent risks. A dive computer considerably increases diving safety, but it does not eliminate the remaining risk of serious injury or death caused by decompression sickness, oxygen toxicity, or other inherent risks of scuba diving.

You should not use this SYMBIOS HUD if you are not aware of or if you do not accept those risks.

In this manual, the following three precautionary messages are used: WARNING, CAUTION, and NOTICE symbols provide users with necessary information about potential hazards and proper procedures.

WARNING

WARNING statements describe potentially hazardous situations which, if not avoided, could result in serious injury or even death.

CAUTION

CAUTION indicates a hazardous situation which, if not avoided, could result in minor or moderate injury.

NOTICE

NOTICE statements are used to provide important information regarding installation, operation, maintenance, performance, general important tips, or instructions for a procedure or situation that, if not performed properly, might cause damage to the device but is unrelated to physical injury.

1.2 Warnings

WARNING

Before using the SYMBIOS HUD, read the manual in its entirety to familiarize yourself with all of the functions of the device.

WARNING

Do not use SYMBIOS HUD if it shows any signs of damage or malfunction. Contact HALCYON or an authorized repair center.

WARNING

Before using SYMBIOS HUD, you must have successfully completed a course in scuba diving and you must have knowledge about the potential risks and hazards of scuba diving.

WARNING

Even if you follow dive tables or a dive computer, the risk from decompression sickness (DCS) or oxygen toxicity cannot be totally eliminated. DCS and oxygen toxicity risk profiles depend on physiological conditions which can vary from day to day. The SYMBIOS HUD cannot account for these variations.

WARNING

We strongly advise that you stay within the exposure limits provided by the instrument to minimize the risk of DCS.

WARNING

No decompression algorithm can provide a guaranteed safe decompression. It is your responsibility to be trained, dive safely, carry backup tables and instrumentation, and compare any decompression schedules generated with the SYMBIOS HUD against established diving tables.

WARNING

Do not ignore warning signs and indicators on the SYMBIOS HUD. This may result in serious injuries or death.

WARNING

You should never share the SYMBIOS HUD with other divers. Always use the same dive computer for repetitive dives. The SYMBIOS HUD features a built-in memory function that keeps track of your diving history. Substituting the SYMBIOS HUD between a series of repetitive dives may result in incorrect decompression calculations.

WARNING

Do not fly or travel to high altitudes while the NO FLY indication remains active. Flying while the SYMBIOS HUD displays NO FLY can result in serious injury or death.

WARNING

If you omit one or more decompression stops, a symbol will indicate the current ceiling to which you should descend. If you continue to ignore these warnings, there is no additional ERROR or LOCKOUT. Do not ignore these warnings. Decompression stops are your responsibility and must be performed for your safety.

WARNING

Always dive with backup instruments: depth gauges, pressure gauges, dive watches, or backup dive computers. While planning a dive with the SYMBIOS HUD, it is recommended that you have access to decompression tables.

WARNING

Contact your instructor or authorized dealer before diving with the SYMBIOS HUD

if you do not fully understand how to use it or if you have any questions.

! WARNING

Do not exceed the limits of your training/certification level.

! WARNING

Always carry and frequently check a backup pO₂ monitoring device.

! WARNING

Always carry and frequently check a backup dive computer.

! WARNING

Before diving, consult a physician regarding your fitness to dive.

! WARNING

In recreational diving, do not dive with a pO₂ > 1.4 bar/ATA. Diving with a high pO₂ may lead to O₂ intoxication.

Never dive with a pO₂ > 1.6 bar/ATA. Diving with a pO₂ > 1.6 bar/ATA will lead to O₂ intoxication.

! WARNING

NITROX diving requires proper training. Do not dive with NITROX without a NITROX certification.

! WARNING

TRIMIX diving requires proper training. Do not dive with TRIMIX without a TRIMIX certification.

! WARNING

Do not use breathing gases other than air, including hypoxic TRIMIX breathing gases, with an O₂ fraction of less than 20% unless you have been properly trained in using

those gases or unless you have a TRIMIX certification.

! WARNING

Do not violate the ceiling depth during decompression. In order to avoid doing so by accident, stay slightly below the ceiling depth. Staying deeper than the required ceiling depth will increase the total time to surface.

1.3 Installation



The SYMBIOS HUD is mounted directly onto a diving mask.



Mask front view

A support is clamped onto the frame of a diving mask.



Mask rear view



The SYMBIOS HUD support allows for simple adjustment by containing two ball joints that accommodate divers' unique eye positioning.

The SYMBIOS HUD is held by a clamp. Use the attachment point of the SYMBIOS HUD to secure the SYMBIOS HUD onto the diving mask.

NOTICE

Washers with different thicknesses or a combination of those are used to adjust the clamp to the size of the frame. 1 mm, 2 mm, and 4 mm washers are included in the package.

NOTICE

The support cannot be installed on all diving masks. If you are not sure if the support fits on your mask, please contact your local dive shop.

! CAUTION

Always use a secondary attachment method to secure your SYMBIOS HUD to your diving mask (e.g., nylon fishing line).

1.4 Operation

Powering On

When the SYMBIOS HUD is not in use, it is in standby mode. In standby mode, the display remains off to minimize power consumption.


Press and release the button A or B to activate the computer.

The SYMBIOS HUD will automatically power off and switch into standby mode if it is not operated while on the surface or has not

received wireless data from a CCR for more than two minutes.

Two-Button Operation

Two tactile push buttons are used to operate the SYMBIOS HUD with short and long presses of the buttons. Use a short press to switch between screens, navigate in a menu, or increment or decrement user settings. Use a long press to confirm selections, enter the main menu, or activate a user-selectable custom function. Within the menu, the long press functions are indicated in boxes on top and bottom of the screen. Long button presses have different functions.

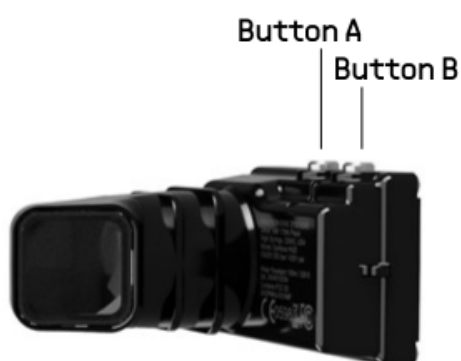

During a dive, the buttons function as follows:

- Short press button A to toggle between different information screens.
- Long press button A to access the menu.
- Short press button B to toggle the custom field.
- Long press button B to perform the custom function set in MENU → SYSTEM → CUSTOM FUNC.
- Long press both buttons at the same time to acknowledge and reset various warnings and alarms.

Custom Field

The information presented in the custom field is dependent on the dive mode. You can select some parameters to be shown in the custom field (left lower field), including:

- Tank pressure of selected gas
- Tank pressure T1 – T4 (only available if a tank pod is paired to T1 – T4, respectively)
- ASC – Ascent speed in m/ft per min
- BAT – Remaining battery charge in % or volts (Depending on the operation mode, this can include the battery state of the Symbios CCR and the Greenflash™ digital oxygen sensor)
- CNS – Central Nervous System O₂ Toxicity in %
- AVG – Average depth
- COMP – Compass heading in °
- TEMP – Temperature
- GF Now – Current Gradient Factor
- GF Surf – Gradient Factor if the diver instantaneously surfaces
- Ceiling – The depth ceiling that the diver can ascend to without depth rounding
- Gas Density – The density of the breathing gas
- CCR FO₂ – Fraction of oxygen currently in the CCR breathing loop
- CCR Dil PO₂ – Partial pressure of oxygen in the diluent at the current depth
- CCR SP – CCR setpoint for oxygen
- SCRUBBER – Usable time remaining of the CO₂ absorbent material in a CCR
- TTS+5 – The projected Time to Surface if the diver remains at the same depth for another five minutes
- TRIM – Diver's trim in ° (requires a Symbios Tank Pod)
- Lamp RRT – Not currently available
- Lamp SOC – Not currently available
- NF – No Fly time (Only displayed on surface after a dive and while there is no fly time remaining)

Custom Function

Press and hold button B to perform the predefined custom function. You can preset this custom function by navigating to MENU → SYSTEM → CUSTOM FUNC. The following functions are available:

Off (No Function)


Start/Reset the stopwatch

Select best gas (this is calculated according to the gas table and the maximum pO_2)

Save waypoint (only available when a wireless GPS signal is received)

BO/SP Low/SP Hi: When in CCR FSP mode, the HUD switches between Bailout (OC), low setpoint, and high setpoint.

1.5 Surface Mode

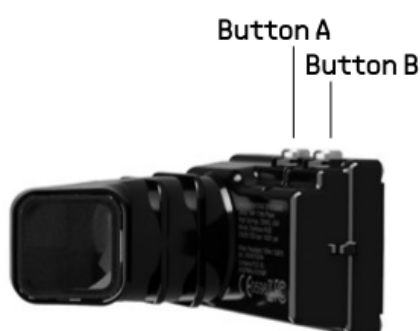

On the surface, the SYMBIOS HUD will typically remain in standby mode to minimize power consumption. In standby mode, a fully charged battery can last as long as six months. However, you should plan to supply a maintenance charge with long-term storage.

Press and release either button A or B to activate the device.



The pictured display (OC mode) shows:

- The compass (top)
- The maximum depth and time of the last dive (under compass)
- Information about the gas used on the last dive (under depth)
- The Surface Interval (SI) (under time)
- The pressure of the breathing gas (bottom left)
- The ascent rate indicator (bottom right)

1.6 Care and Maintenance

The SYMBIOS HUD is built from high-quality, seawater-resistant materials. The SYMBIOS HUD is designed to withstand diving in harsh conditions. However, divers should still protect the SYMBIOS HUD from mechanical shock, excessive temperatures, chemicals, and mechanical tampering.

Long term maintenance and/or repair actions are not required.

NOTICE

After diving, rinse the SYMBIOS HUD in freshwater to avoid corrosion.

NOTICE

Before connecting the SYMBIOS HUD to a USB cable, ensure that the USB connector on the SYMBIOS HUD is clean and dry. Failure to do so may lead to corrosion of the contacts.

CAUTION

Protect the SYMBIOS HUD from mechanical shocks and during transportation.

CAUTION

Do not try to open or repair the SYMBIOS HUD. The SYMBIOS HUD does not contain any user-serviceable parts. Service may only be performed by HALCYON or by an authorized service center.

CAUTION

Inspect the SYMBIOS HUD for mechanical damage and cracks before and after each dive to ensure proper working condition.


NOTICE

Failure to observe the above precautions voids the warranty along with any product-related liability of Halcyon.

Charging and USB Connection



The SYMBIOS HUD features a USB port for charging.

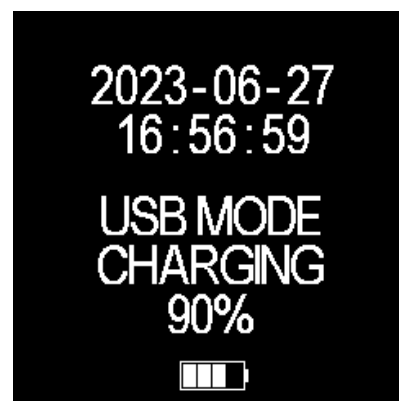

The SYMBIOS HUD will display a charging screen when it is plugged in.

You may charge the SYMBIOS HUD using any USB-compatible power source.

When connected to a PC, the SYMBIOS HUD will also appear as a removable drive on the PC and can be accessed like a USB drive.

WARNING

If the battery indicator flashes red during a dive, the battery level is low and the dive computer may soon switch off or perform a reset. After a reset, dive data, depth, dive time, and decompression obligations will be incorrect.

WARNING

Do not dive when the SYMBIOS HUD battery indicator is red. The dive computer might run out of battery during the dive. In such a case, the SYMBIOS HUD may give incorrect depth readings, incorrect decompression data, or may shut off completely. In case of a red battery indicator, recharge the SYMBIOS HUD before the next dive.

WARNING

Never fully discharge the SYMBIOS HUD; full discharge may damage the lithium ion rechargeable battery.

⚠ WARNING

If the battery is completely discharged, the dive computer may reset and lose all decompression information. If a reset occurs between repetitive dives, be aware that the SYMBIOS HUD loses decompression data and compartment inert gas pressure data from previous dives; thus, decompression readings and calculations for any following dives should be considered incorrect.

NOTICE

After a dive, before connecting the cable, rinse the SYMBIOS HUD in freshwater. Make sure that the USB connector is clean and dry before connecting the USB cable.

NOTICE

Do not disassemble or remodel any cables or connectors. Use only the original USB cable supplied with the SYMBIOS HUD. Check compatibility before use.

NOTICE

Use only a clean and dry USB cable. Clean and dry the connector surfaces of the cable before use.

NOTICE

If the SYMBIOS HUD is completely discharged, charge the device for at least three hours before use.


NOTICE

Before using the SYMBIOS HUD for the first time, charge the device for at least three hours.

NOTICE

Charge the SYMBIOS HUD with a USB power source with a nominal output of 5V and at least 500 mA of electrical current.

2 Settings

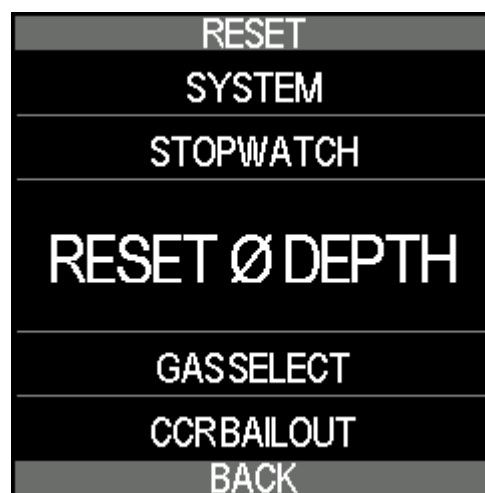

The SYMBIOS HUD has an intuitive menu which allows you to change settings quickly.

NOTICE

Press and hold button A to access the menu.

NOTICE

Press and release button A or B to navigate in a menu or to increment or decrement a setting.

NOTICE

Within the menu, the long press functions of both buttons are indicated in boxes on the top and bottom of the menu.

Press and hold button A to perform the function indicated on top of the menu. Press and hold button B to perform the function indicated on the bottom of the menu.

2.1 Menu

Long press button A to enter the menu.

Once in the menu:

Short press and release button A to navigate up in the menu.

Short press and release button B to navigate down in the menu.

Long press button A to perform the function indicated on the top row of the screen.

Long press button B to perform the function indicated on the bottom row of the screen.

STOPWATCH

Start/Reset the stopwatch

RESET AVERAGE DEPTH

Reset the average depth

GAS SELECT

Select an active gas from the gas table

CCR BAILOUT

AUTO

Automatically switch between Bailout and Closed Circuit mode (only available on the Symbios CCR with an automatic BO/CC sensor)

CC

Closed Circuit mode (overrides auto setting)

BAILOUT

Bailout mode (overrides automatic setting)

CCR SETPOINT (only for CCR FSP mode)

SETPOINT HIGH

Setpoint High for constant pO_2 deco calculation

The pO_2 can be set between 1 and 1.6 bar

SETPOINT LOW

Setpoint Low for constant pO_2 deco calculation

The pO_2 can be set between 0.5 and 0.9 bar/ATA

HEADING

Select or edit up to three headings

WAYPOINT

Select or save up to 64 waypoints (requires a GPS signal)

SETTINGS

DIVE MODE

OC

Open Circuit diving mode

CCR

Closed Circuit Rebreather diving mode using a compatible Symbios CM eCCR

CCR FIX SP

Closed Circuit Rebreather diving mode with Fixed Setpoints

SIDEMOUNT

Sidemount diving mode

BOTTOM TIMER

Bottom timer mode

(In this mode, the SYMBIOS HUD does not perform deco calculations.

After diving with the bottom timer mode, users cannot enable other dive modes for a period of 24 hours.)

EDIT GASES

MODIFY

EDIT

Allows diver to edit the O_2 and He fraction of the selected gas

ENABLE/DISABLE

Enables or disables the selected gas

Only enabled gases can be selected in MENU → SELECT GAS

PRESET

Allows diver to select a gas from the pre-programmed gas library

GFL/GFH

Allows the diver to select or modify the Gradient Factor Low and Gradient Factor High (the default setting is 45/80)

OC PO₂ DECO

Maximum allowed oxygen partial pressure for decompression and gas switch calculations in open circuit diving mode

OC PO₂ BOTTOM

Maximum allowed oxygen partial pressure for MOD calculation of the bottom gas (Bottom gas is defined as the gas with the lowest oxygen fraction within the enabled gases for the dive.)

CCR SETTINGS**PO₂ SENSORS (only for Symbios CM eCCR)**

Enabling or disabling O₂ sensors to include/exclude them from decompression calculations

SCRUBBER TIMER

Shows the remaining scrubber time in minutes and allows the diver to reset the timer

ENABLE/DISABLE

Enables or disables the scrubber timer

TIMER MAX

Sets the max allowable use time of the scrubber

PO₂ SETPOINT (only in CCR FSP mode)

Sets the pO₂ setpoint high and setpoint low that will be used for the decompression calculation while diving in CCR FSP mode

TRIM SENSOR**HORIZONTAL**

To detect trim, the dive computer must be paired with a combined tank. pressure/trim sensor and the sensor must be pressurized. Bring the diving tank into a horizontal position where the tank(s) is/are lying horizontally on the back.

Use this menu item to perform a horizontal calibration of the trim sensor.

VERTICAL

To detect trim, the dive computer must be paired with a combined tank pressure/trim sensor and the sensor must be pressurized.

Bring the diving tank into a vertical position where the tank(s) is/are standing vertically with the tank valves up.

Use this menu item to perform a vertical calibration of the trim sensor.

PAIRING**TANK POD****TO GAS**

Pair a tank pod with an active gas from the gas table

TO NUMBER

Pair a tank pod to T1, T2, T3, or T4 (independent of the gases in the gas table)

CCR INTERFACE

Pair a SYMBIOS eCCR interface

GPS

Pair a GPS buoy

COMPASS

Pair with an external compass module (This feature will be enabled when the external compass module becomes available.)

TRIM SENSOR

Pair with a trim sensor

DPV

Pair with a compatible Diver Propulsion Vehicle (DPV)

GAS ANALYZER

Pair with a SYMBIOS gas analyzer (This feature will be enabled when the SYMBIOS Gas Analyzer becomes available.)

LOGBOOK

This submenu contains all previous dives. Select a dive to display information including the depth and temperature profile or the pO₂ sensor signals in CCR mode.

SYSTEM**BRIGHTNESS**

Display brightness (Default setting is 5)

TIME

Set time

DATE

Set date

UTC

Set UTC time zone

SAFETY STOP

Enable/disable a safety stop

(If enabled, at each dive with a maximum depth >10 m/30 ft, the diver will be prompted to do a 3 minute safety stop at a depth between 3-6 m/10-16 ft.)

LAST STOP

Allows the user to select the depth of the last decompression stop

VIB ALARMS

Enable/disable vibration alarms

COMP CAL

Calibration of the internal compass
(Activate this menu item and then move the computer in a figure 8 in front of you.)

COMP DECLIN

Setting of the compass declination

LANGUAGE

Language setting

UNITS

Metric/imperial units

DENSITY

EN13319

Depth calculation is based on EN13319 where 1 bar pressure increase equals 10 m/33 ft.

SEA WATER

FRESH WATER

STYLE

CLASSIC

MODERN

SLEEP

Time after which the dive computer switches into sleep mode (2 - 59 minutes)

DIVE TIMEOUT

Time after which the dive computer switches from dive mode to surface mode

ORIENTATION

Change the button orientation for use on the left, right, or top sides

WIRELESS SCRN

OFF

The wireless data screen is inactive

ADDITIONAL

Enables a wireless screen that shows information from all transmitters in close vicinity that are NOT paired with the dive computer

(This is the preferred setting to monitor the tank pressure of a dive buddy.)

ALL

Enables a wireless screen that shows information from all transmitters in the close vicinity

BUDDY SCREEN

Enable or disable the buddy screen. When the buddy screen is enabled, information from a SYMBIOS eCCR that is not paired with the user's HUD will be presented when the unit is in reception range.

DECO SCRN

Enable or disable the deco screen which shows detailed decompression information including deco stops, time and depth, and ceiling

On the Custom Field (lower left field), the user-selected information labels appear

GF CHART

Enable or disable the GF screen which shows a graphical representation of the 16 compartments used in the decompression algorithm and their respective gas loading in real time

DEPTH CHART

Enable or disable the depth chart screen which presents a graphic representation of the dive profile in real time

TRAINING

Enable or disable the training simulation function which allows users to create and perform simulated decompression stops

CUSTOM FUNC

Setting the default function of "Press and hold the B button"

BEST GAS

Press and hold button B to confirm the suggested gas switch

STOPWATCH

Press and hold button B to start/reset the stopwatch

WAYPOINT

Press and hold button B to save a waypoint
(This requires a GPS signal)

BAILOUT/SETPOINT SET (only in CCR FSP mode)

Press and hold button B to alternate
between Low Setpoint/High
Setpoint/Bailout when using CCR FSP mode

OFF**CF DEFAULT**

Set the default item for the custom field
(lower field on the left side)

NO/DEFAULT

Deactivated

ACTIVE GAS

Custom field shows active gas and tank
pressure of active gas

T1

Custom field shows pressure of tank
transmitter T1

T2

Custom field shows pressure of tank
transmitter T2

T3

Custom field shows pressure of tank
transmitter T3

T4

Custom field shows pressure of tank
transmitter T4

CF CONTENT

Enables or disables user-selected items
displayed on the custom field (lower left
field on the screen)
(Please note that the available options are
dependent on the dive mode.)

AVERAGE DEPTH**BATTERY SOC**

State of charge of the HUD battery

CNS**TEMPERATURE****ASCEND SPEED****PO₂**

When in bottom timer mode and with a tank
pod paired to a gas, the HUD will display the
pO₂ of the selected gas.

TIME

When in bottom timer mode, the HUD will
display the date and time of the day.

HEADING**GF NOW**

Current gradient factor

GF SURFACE

Hypothetical gradient factor if the diver
surfaced at this point of the dive

GAS DENSITY**CCR FO₂**

O₂ fraction of the breathing gas in the loop

TIME / DATE

Only available in bottom timer mode

DILUENT PO₂

PO₂ of the diluent gas at the current depth

SETPOINT

Setpoint of the pO₂ controller

CEILING:

The depth ceiling that the diver can
ascend to without depth rounding

TTS+5:

The projected Time to Surface if the
diver remains at the same depth for
another five minutes

LAMP SOC

State of charge of the forthcoming
Halcyon dive lights

LAMP RRT

Remaining run time of the
forthcoming Halcyon dive lights

SYSTEM INFO**SERIAL ID**

Serial number of your SYMBIOS HUD

FIRMWARE

Firmware number of your SYMBIOS
HUD

BUILD DATE

Build date of the firmware of your
SYMBIOS HUD

BT CODE

Six-digit BT code of your SYMBIOS
HUD

RESET COMPTS

Reset the compartments of your
SYMBIOS HUD

(Press and hold both buttons for five seconds to confirm.)

RESET SETTINGS

Reset the settings of your SYMBIOS HUD

(Press and hold both buttons for five seconds to confirm.)

RESET SYSTEM

Reset the SYMBIOS HUD

(This resets neither the settings nor the compartments. Press and hold both buttons for five seconds to confirm.)

DIAGNOSIS

Information about the sensors of your HUD device

CCR DIAGNOSIS

Present operational condition of SYMBIOS eCCR that is paired to the HUD. Affected components will be shown in red.


SLEEP

On the surface, long press button A to put your HUD into sleep mode.

2.2 Select a Gas

You can select your diving gas using the SELECT GAS menu item. Alternatively, you can switch to the prompted gas during the dive by pressing and holding button B. For this option to be available, you must select BEST GAS as the custom function of button B.

Any of the gases activated in the gas table can be selected.

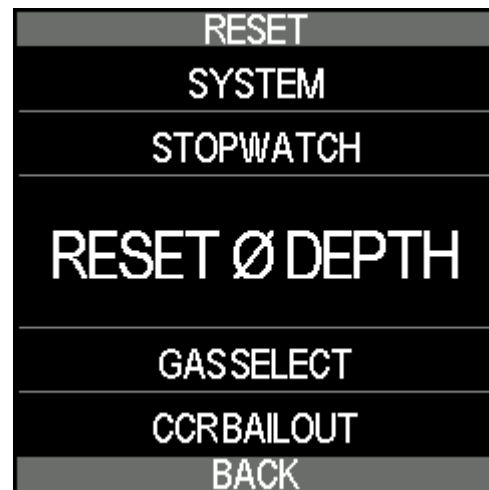

To select a gas from one of the main screens:

Long press button A to enter the menu.

Short press button B to navigate to menu item SELECT GAS.

Long press button A to open the SELECT GAS MENU.



Within the SELECT GAS menu:

Short press either button to navigate between five open circuit gas and three diluent gas settings.

Long press button A to select one gas setting.

Long press button B to go back to the menu.

Divers can only select gases that are activated. Activate a gas during the dive via the GAS TABLE menu item.

2.3 Edit a Gas Setting from the Gas Table

To edit the contents of the gases in the gas table or to activate and deactivate gases, navigate to the GAS TABLE menu found in SETTINGS.



Short press either button to navigate to the gas entry you want to modify. Long press button A to modify a gas entry. Long press button B to return to the menu.



Short press either button to navigate to the EDIT, ENABLE/DISABLE, or PRESET options in the MODIFY menu.

Long press button A to select the highlighted function in the center of the screen. Long press button B to return to the menu.

Editing Gas Content



To edit the contents of a gas in the gas table, short press either button to increment or decrement a digit. Long press button A to set the digit and move to the next digit. Long press button B to delete the gas entry.

Enabling/Disabling a Gas

Enable, disable, or select a gas from a pre-programmed gas library in the EDIT GAS menu.

Only enabled gases can be selected in the SELECT GAS menu.

Presets

The PRESET menu includes the following pre-programmed gases:

- TX10/85
- TX10/50
- TX15/55
- TX18/45
- NX21/35

- NX21(AIR)
- NX32
- NX35
- NX50
- NX80
- NX99 (O₂)

⚠ WARNING

Do not change gas settings unless you are trained in NITROX, TRIMIX, or mixed gas diving.

2.4 Pairing

Wireless Interface

The SYMBIOS HUD features an innovative wireless receiver capable of receiving data from multiple sources. Those include:

- SYMBIOS Tank Pod
- SYMBIOS pO₂ Transmitter
- SYMBIOS pO₂ Transmitter, P-Port version
- SYMBIOS CM ECCR
- SYMBIOS GPS Buoy
- SYMBIOS wireless OEM interface



To pair wireless devices, navigate to Menu → SETTINGS → PAIRING.

Pairing a SYMBIOS Tank Pod



Pairing a SYMBIOS Tank Pod with Gas in the Gas Table

Pair the SYMBIOS Tank Pod in MENU → SETTINGS → PAIRING → TANK POD.

1. Install the SYMBIOS Tank Pod on a first stage. The SYMBIOS Tank Pod is suitable for tank pressures up to 300 bar/4,350 psi.
2. Attach the first stage to the tank and open the tank valve.
3. Wait approximately 15 seconds for the transmitter to switch on. Ensure that the SYMBIOS HUD and the SYMBIOS Tank Pod are in close proximity (ideally <40 cm/16 in).
5. Navigate to MENU → SETTINGS → PAIRING → TANK POD → TO GAS.
6. Short press either button to navigate to and select the appropriate gas entry for the SYMBIOS Tank Pod.
7. Long press button A to select a gas entry.
8. Long press button A to start pairing.



If the pairing process is successful, the SYMBIOS HUD will display the tank pressure.

If you have any trouble pairing please verify you are not trying to pair a given transmitter to multiple gases or transmitter numbers. This is the most common cause of pairing problems. Unpair from all other gases/transmitters and try the pairing process again.

To unpair the SYMBIOS Tank Pod, navigate to MENU → SETTINGS → PAIRING → TANK POD → TO GAS. Short press either button to select the gas you want to unpair. Long press button B to unpair the SYMBIOS Tank Pod.

Pairing a SYMBIOS Tank Pod Independently from the Gas Table

You may pair a SYMBIOS Tank Pod independently of the gas table. A SYMBIOS Tank Pod can be paired with either T1, T2, T3, or T4.

To pair a SYMBIOS Tank Pod :

1. Install the SYMBIOS Tank Pod on a first stage. The SYMBIOS Tank Pod is suitable for tank pressures up to 300 bar/4,350 psi.

2. Attach the first stage to the tank and open the tank valve.
3. Wait approximately 15 seconds for the transmitter to switch on. Ensure that the SYMBIOS HUD and the SYMBIOS Tank Pod are in close proximity (ideally <40 cm/16 in).
4. Navigate to MENU → SETTINGS → PAIRING → TANK POD → TO NUMBER.
5. Short press either button to navigate to T1, T2, T3, or T4.
6. Long press button A to select one of the menu entries.
7. Long press button A to begin pairing.

Pairing the Trim Sensor

The SYMBIOS Tank Pod is equipped with a high-resolution, 3-axis accelerometer which assesses diver trim.

After pairing a SYMBIOS Tank Pod, pair the trim sensor to either a gas entry in the gas table or an entry from the number table (i.e., T1 – T4).

1. Ensure that the SYMBIOS Tank Pod is pressurized and transmitting tank pressure data.
2. Navigate to MENU → SETTINGS → PAIRING → TRIM SENSOR.
3. Press and hold the top button to begin pairing.



The diver trim is indicated in the custom information field.

Calibrating the Trim Sensor

After pairing a trim sensor or changing the orientation of the SYMBIOS Tank Pod with respect to the tank, calibrate the trim sensor.

First, perform a horizontal calibration:

1. Pressurize the SYMBIOS Tank Pod and place the dive tank in a horizontal position.
2. Navigate to MENU → SETTINGS → TRIM SENSOR → HORIZONTAL.
3. Long press button A to perform the horizontal calibration.

In the second calibration step, perform a vertical calibration:

1. Orient the tank vertically with the valve up.
2. Navigate to MENU → SETTINGS → TRIM SENSOR → VERTICAL.
3. Long press button A to perform the vertical calibration.

NOTICE

A SYMBIOS Tank Pod can only be paired with one entry in the menu. Before pairing a SYMBIOS Tank Pod with a new gas entry, unpair it from the SYMBIOS HUD.

⚠ WARNING

Even when using a SYMBIOS Tank Pod, always use a backup tank pressure gauge. Check the backup tank pressure gauge at regular intervals.

NOTICE

Complete a calibration each time the orientation of the SYMBIOS Tank Pod

changes with respect to the tank.

Otherwise, without a re-calibration, the tilt reading may be incorrect.

Pairing a SYMBIOS CM eCCR



To pair the SYMBIOS HUD with a SYMBIOS CM eCCR:

1. Navigate to MENU → SETTINGS → PAIRING → CCR INTERFACE.
2. Turn on the SYMBIOS CM eCCR.
3. Press and hold the top button to start pairing.

NOTICE

You must calibrate the O₂ sensors after pairing the SYMBIOS CM eCCR Transmitter. To complete calibration, follow the instructions on the user manual of the SYMBIOS CM eCCR

NOTICE

If a wireless transmitter is too far from the SYMBIOS HUD and data cannot be received, the values will be grayed out on the display.


⚠ WARNING

Always use backup instruments for your SYMBIOS pO₂ Transmitter or SYMBIOS Tank Pod.

2.5 Compass Calibration

To perform a compass calibration, go to MENU → SYSTEM → CAL COMPASS.

The compass calibration takes approximately two minutes. Within these two minutes, move the SYMBIOS HUD in a figure 8 in front of you.

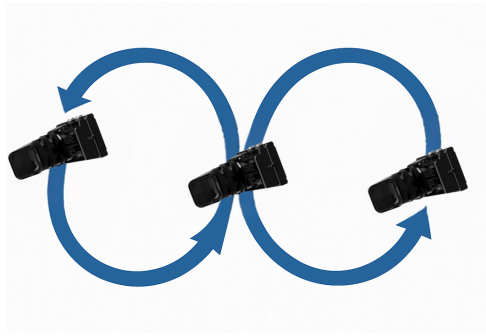

After the calibration, check the compass heading. If the compass heading is incorrect, recalibrate the HUD. If the compass heading is still incorrect, there may be magnetic disturbances at your location. Go to a different location (outside a building and distant from electric power lines) and recalibrate the HUD.

3 Diving

You can use the SYMBIOS HUD for recreational or technical diving: air, NITROX, or TRIMIX open circuit diving and closed circuit rebreather diving with a constant pO_2 setpoint.

You can also use the SYMBIOS HUD as a communication hub for the SYMBIOS Cm eCCR. The SYMBIOS HUD offers live pO_2 sensor monitoring and rebreather operating status information.

The SYMBIOS HUD also offers support for sidemount diving (paired with SYMBIOS TANK Pods) and can operate in Bottom Timer mode (where no decompression calculations are performed).

Dive mode is automatically activated as soon as you reach a depth >1 m/3 ft. After surfacing and after a two-minute timeout, surface mode is activated. You can adjust the time interval to enter surface mode.

During diving,

- Short press button A to switch between different screens.

- The lower left field on the screen is the custom field. Choose the default item shown in this field in MENU → SYSTEM → CF DEFAULT.

- Short press button B to switch between different items in the user-selectable custom field.

After 60 seconds, the item in the custom field will automatically switch back to the preset field in MENU → SYSTEM → CF DEFAULT unless the user has selected the No Default option in the CF Default menu.

- Long press button A to enter the menu.

- Long press button B to perform the custom function (MENU → SYSTEM → CUSTOM FUNC).

In open circuit diving mode or closed circuit bailout mode, the default setting for this function is to confirm a suggested gas switch.

In CCR FSP mode, the default setting for this function is to cycle the HUD through Bailout, Closed Circuit Setpoint Low, and Closed Circuit Setpoint High.


In bottom timer mode, the default setting for this function is to start/reset the stopwatch.

The SYMBIOS HUD features different screens. Short press button A to switch between screens.





This is the first screen. The current depth is 22.8 m, dive time is seven minutes, remaining tank pressure is 138 bar, and remaining no-decompression limit is 13 minutes. The diver is breathing air (NX21). The compass heading is indicated at the top of the screen.

Short press button A to switch between different screens.

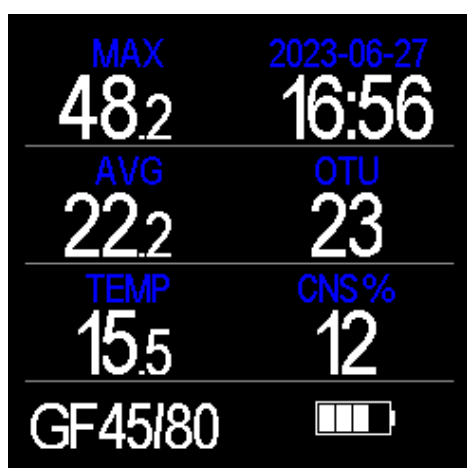

The second screen displays auxiliary data. You can enable additional screens (to, for instance, show wireless information or a detailed deco schedule) in the menu.

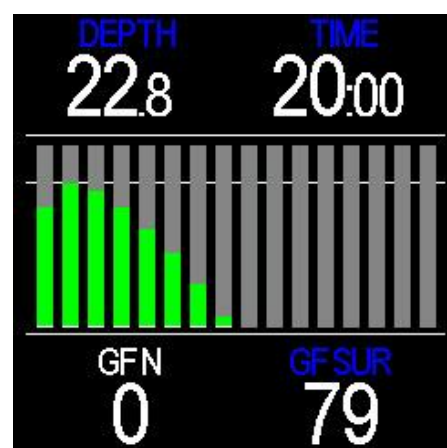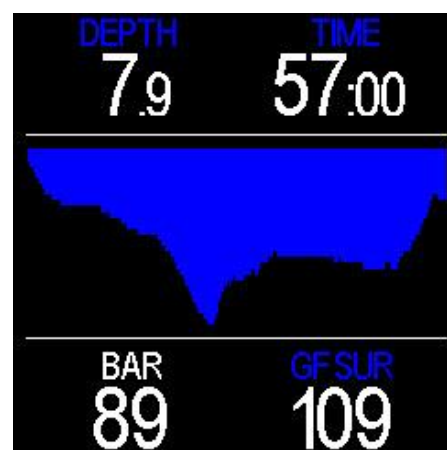

The real time depth profile screen (top) and the tissue compartments gas loading screen (bottom) are two additional screen options available.

! WARNING

The risk of decompression sickness (DCS) or oxygen toxicity for any dive profile cannot be totally eliminated—even if you follow dive tables or a dive computer. DCS and oxygen toxicity risk profiles also depend on physiological conditions which can vary from day to day.

The SYMBIOS HUD cannot account for these variations.

! WARNING

We strongly advise that you stay within the exposure limits provided by the instrument to minimize the risk of DCS. However, even if you stay within recreational limits and the

no-decompression limits given by this dive computer, DCS symptoms may still occur.

WARNING

Before diving, consult a physician regarding your fitness to dive.

WARNING

In recreational diving, do not dive with a $pO_2 > 1.4$ bar/ATA. Diving with a high pO_2 may lead to O_2 intoxication.

Never dive with a $pO_2 > 1.6$ bar. Diving with a $pO_2 > 1.6$ bar/ATA will lead to O_2 intoxication.

WARNING

Do not dive deeper than what your current diving qualification allows.

WARNING

NITROX diving requires proper training. Do not dive with NITROX without a NITROX certification.

WARNING

Besides the decompression stops, there are no additional mandatory safety stops or error messages displayed when you violate the decompression ceiling and time or the recommended ascent rate.

WARNING

Do not violate the ceiling depth during your decompression. In order to avoid doing so by accident, you should stay slightly below the ceiling depth. Staying deeper than the required ceiling depth will increase your total time to surface

WARNING

Do not use breathing gases other than air, unless you are certified in NITROX or TRIMIX diving.

WARNING

Do not use breathing gases other than air, in particular hypoxic TRIMIX breathing gases with a O_2 fraction of less than 20%, unless you have a TRIMIX certification.

3.1 Preparations Before the Dive

Switch on the SYMBIOS HUD before diving and complete all necessary settings changes on the surface. Check the SYMBIOS HUD for damage before diving. Before entering the water, check:

- Battery level
- Conservatism (gradient factors) settings
- Gas settings
- Time and date
- Units (imperial or metric)

Switch on the SYMBIOS HUD before you enter the water.

WARNING

Before each dive, check the battery power and recharge the battery if necessary. Recharge the battery when the computer has not been used for an extended time. Low temperatures can affect battery performance. Pay special attention to the charge level of the battery during cold-water dives.

WARNING

Before each dive, verify that the SYMBIOS HUD settings are correct.

WARNING

When using breathing gases other than air, analyze the breathing gas before the dive.

Verify that the fractions in the gas table are correctly set.

WARNING

Set the SYMBIOS HUD to your preferred measurement units (imperial or metric).

3.2 Decompression Model

The SYMBIOS HUD calculates no-decompression times and decompression stops, depth, and duration using a mathematical decompression model which estimates the inert gas uptake and elimination during diving. The SYMBIOS HUD uses the Bühlmann ZH-L16C dataset. The model uses 16 hypothetical compartments for nitrogen and 16 for helium to estimate the inert gas loading of the body's tissues during a dive.

Gradient factor (GF) allows divers to customize the algorithm. Using the GF concept, divers can reduce the maximum allowable compartment gas loading to a percentage of the maximum permissible loading according to the original Bühlmann ZH-L16 model. In other words, a GF below 100 results in shorter no-decompression times and longer decompression schedules and is more conservative than the original algorithm.

There are two GFs. GF High limits the maximum allowable compartment inert gas loading. GF Low is only relevant for decompression diving. It reduces the maximum allowable compartment gas loading at depth. A low GF Low setting results in deeper decompression stops.

The SYMBIOS HUD features a very precise pressure sensor which can also be used as an altimeter. This allows the SYMBIOS HUD

to adapt automatically to the reduced atmospheric pressure in altitude diving.

NOTICE

A lower GF High results in shorter No-Decompression Limits.

NOTICE

Diving with a lower GF High reduces the risk of decompression sickness.

NOTICE

GF Low is only relevant when completing dives requiring mandatory decompression stops. A GF Low setting lower than a GF high setting results in deeper stops.

WARNING

Do not change GF settings unless you have proper training in decompression theory, the m-value concept, and gradient factors.

3.3 Time To Surface (TTS) Calculation

The SYMBIOS HUD calculates the Time To Surface (TTS) value based on parameters that affect the decompression calculations of the dive.

These parameters include:

- Inert gas loading at the beginning of the dive
- Dive profile (depth and bottom time)
- Gas used
- Partial pressure of oxygen when in closed-circuit dive modes
- The Gradient Factors selected by the user
- Ascent rate (the SYMBIOS HUD uses an ascent rate of 9 m/29 ft per minute to calculate the TTS)

During the dive, the SYMBIOS HUD assumes that you will use all the gases marked as

active on the gas table to calculate the TTS. If you lose access to any of the gases during the dive, remove the affected gas from the list of active gases in the gas table to ensure an accurate TTS calculation.

3.4 Training Mode

Training mode allows you to create a simulated decompression plan while diving. This allows divers the opportunity to practice decompression stop diving in a real environment while still remaining within the NDL limit.

To enable the training mode, go to MENU → SYSTEM → TRAINING. Once enabled, a menu will be available while diving under the following conditions:

- You are within the No-Decompression Limit

- Depth is shallower than 30 m/100 ft

To create a simulated decompression plan, long press button A to enter the menu and select Training. Choose one of the six simulated dive profiles, and the computer will generate a simulated decompression profile based on your selection and current tissue loading.

3.5 Dive Modes

The SYMBIOS HUD offers different dive modes which can be selected in menu → SETTINGS → DIVE MODE.

You can choose between the following modes:

- OC – Open Circuit Mode, suitable for air, NITROX, and mixed gas diving
- CCR – Closed Circuit Rebreather Mode with pO₂ sensor readout
- CCR FIX SP – Closed Circuit Rebreather Mode with fixed pO₂ setpoints

- BOTTOM TIMER – Bottom timer mode; no decompression calculations are carried out
- SIDEMOUNT – Sidemount diving mode for diving with two separate tanks

NOTICE

In Bottom Timer mode, the dive computer is not performing any decompression calculations or compartment saturation updates.

After using the dive computer in Bottom Timer mode, decompression calculations on repeat dives would be inaccurate. Therefore, after diving in Bottom Timer mode, you cannot change to a different dive mode within 24 hours.

3.6 Open Circuit Diving


Set the SYMBIOS HUD to open circuit diving mode in menu → SETTINGS → DIVE MODE → OC.

Diving with Air (NX21)



This is the main screen during a dive with air (breathing gas NX21). The current depth is 22.8 m and the dive time is seven minutes. The remaining no-decompression limit is 13 minutes. The remaining tank

pressure is 138 bar. The bar graph on the left side visualizes the tank pressure. The range of the bar graph is 0 to 300 bar. The bar graph on the right side displays the ascent speed (range 0 to 18 m/0 to 59 ft per min).

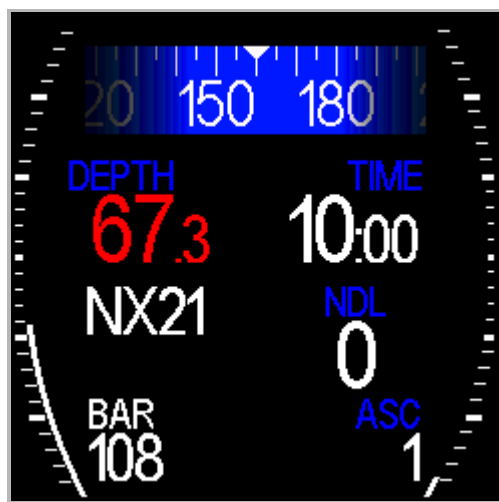

If the pO_2 of the breathing gas exceeds 1.6 bar/ATA or the maximum allowable pO_2 set by the diver, the depth indicator will blink white and red. Set the maximum pO_2 for the bottom gas in menu → SETTINGS → OC PO_2 BOTT.

The remaining no-decompression limit is 0 minutes, and the remaining tank pressure is 108 bar.



The tank pressure is 45 bar and the reading is blinking red and white. If the tank pressure falls below 50 bar, the pressure value will blink red and white. The safety stop timer is also displayed.



The SYMBIOS HUD features a resettable stopwatch. You can activate it with a long press of button B (if the custom function is set to stopwatch) or from the main menu.

Decompression Diving



You may exceed the no-decompression limit during your dive. In this case, the SYMBIOS HUD will also display the decompression stop depth and the time to surface. The decompression stop depth is 6 m, and the estimated time to surface is five minutes. The current ascent rate is 10

m/min (bar on the right side, scale from 0 to 18 m/0 to 59 ft per min maximum).



If you violate the current decompression stop depth, the current decompression stop depth will blink white and red.


Safety Stop Indicator



At the end of the dive, when there are no further decompression obligations, the SYMBIOS HUD proposes a three-minute safety stop at a depth between 3 and 5 m/10 to 16 ft. The safety stop timer counts from 3 minutes to 0, as long as you are at a depth between 3 and 5 meters. If you descend again to 10 m/30 ft depth or more, the safety stop counter will be reset to 3 minutes. The safety stop indicator can be

enabled/disabled in menu → SYSTEM → SAFETY STOP.

Auxiliary Screen

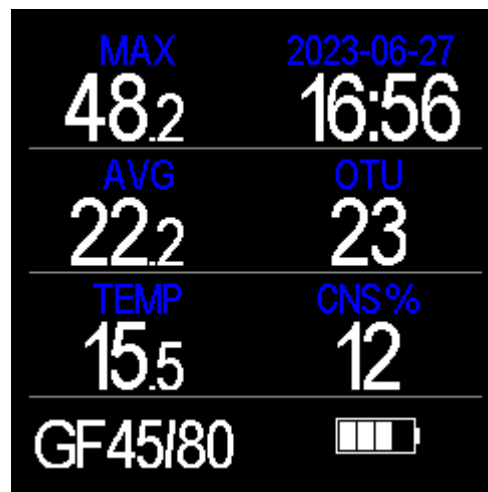

Short press button A to toggle screens. The auxiliary screens provide additional information including maximum depth, current time and date, average depth, OTU, CNS%, and the current temperature. The gradient factor settings and the battery charge status are both displayed at the bottom of the screen.

Diving with NITROX




The SYMBIOS HUD indicates your breathing gas. The current breathing gas is NITROX NX32 containing 32% O₂ and 68% N₂. The remaining tank pressure is 138 bar.

Diving with TRIMIX



The current breathing gas is set to TRIMIX 18/45 containing 18% O₂, 45% He, and 37% N₂.

Gas Switches

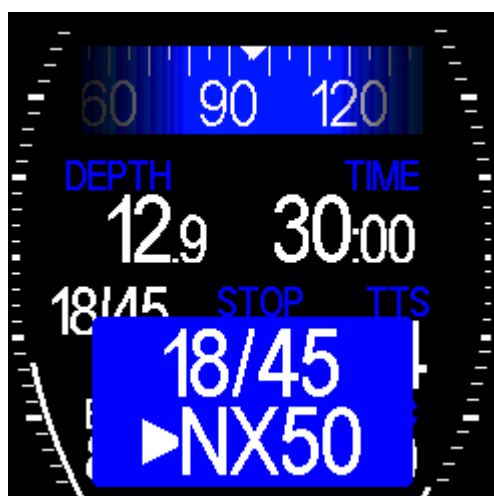


To accelerate decompression, you can use different gas mixes. One gas frequently used for decompression is NITROX 50 (NX50). Before the dive, set the gas table according to the gases you plan to use during the dive (menu → GAS TABLE). The SYMBIOS HUD will automatically calculate the best gas for the current depth based on the max pO₂ selected by you. If the currently selected gas differs from the best, a popup field will prompt you to switch gases.

The gas currently selected is TRIMIX TX18/45. Based on the active gases stored in the gas table, the SYMBIOS HUD proposes NX50 as the best gas. After performing the gas switch, select the correct breathing gas on the SYMBIOS HUD. There are two possible ways to select the best gas:

- Select NX50 in the gas table.
- Long press button B to select the best gas. This, however, requires that the custom function for Press and Hold button A is set to BEST GAS (menu → SETTINGS → CUSTOM → BEST GAS)

Deco Screen

Activate an optional DECO screen in menu → SYSTEM → DECO SCR.N.

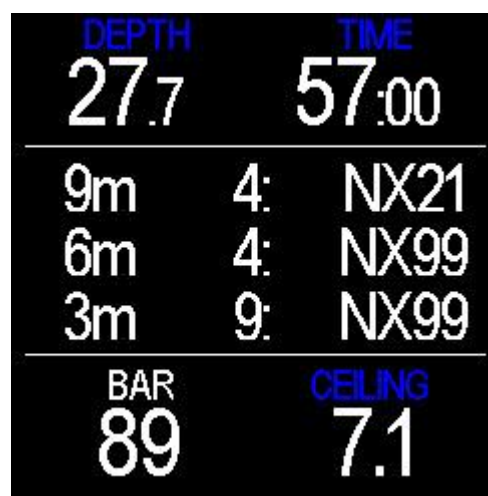


The deco screen shows:

- The current depth and dive time (top)
- The next three deco stops and the best gas available for the stop depth (middle)
- Custom field selected information (bottom left)
- Ceiling depth (bottom right)

Ceiling is the unrounded minimum depth that you can ascend to while still respecting the selected Gradient Factors.

Tissues Loading Screen

Activate an optional tissues loading screen in menu → SYSTEM → GF CHART.

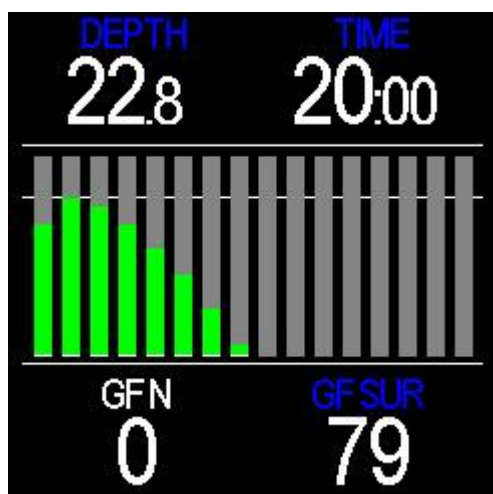


In the tissues loading screen, you can monitor the gas loading of the 16 tissue compartments of the decompression model in real time. The fastest tissue compartment of the model is represented in the far left of the screen while the slowest tissue compartment is on the far right of the screen. If the loading of the tissues has not exceeded the Gradient Factor High set by you (all the tissues are green in color). The line at the top of the screen represents the GF High limit. The short white line within each tissue compartment bar represents the GF NOW value. The GF surface value is displayed on the lower right side.



As you remain at depth, some of the tissue compartments have exceeded the Gradient

Factor High that you set. The tissue compartments that have exceeded the limit are represented in red. The line in the middle of the screen represents the GF High limit.

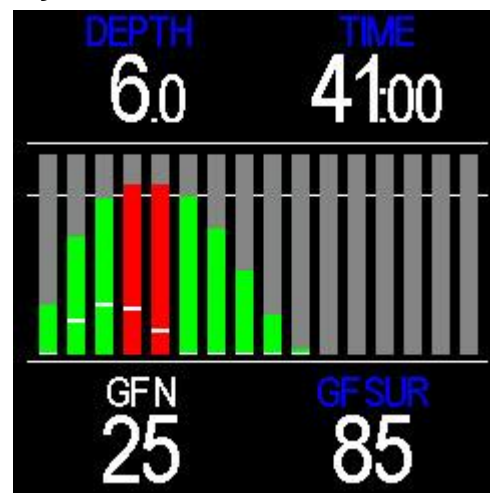

During the ascent and the required decompression stop, the tissue compartments are off-gassing. Given enough time, some of the tissue compartments will fall below the selected Gradient Factor High (represented in green) while other tissue compartments will require more time to off-gas (represented in red). The line near the top of the screen represents the GH High limit. The short white line within each tissue compartment bar represents the GF NOW value.

After the Dive



The SYMBIOS HUD will switch to surface mode after surfacing and a timeout of 2 minutes, unless you have set a longer time in the settings menu or in the Halcyon app.



On the surface, the auxiliary screen displays additional data including the NO FLY timer and the current time and date.

The second and third rows display data from the last dive including average depth, OTU, minimum water temperature, and the current CNS% loading.

The bottom row displays the current Gradient Factor setting and the remaining battery capacity.

The NO FLY timer is also displayed on the custom information field on the main screen.



If you have violated a decompression stop depth ceiling and/or decompression obligations during the dive, the SYMBIOS HUD displays a DECO warning at the end of the dive.



If you have enabled a safety stop (default setting), the maximum depth of the dive was deeper than 10 m/30 ft, and the safety stop was not finished, the SYMBIOS HUD displays a STOP warning.

3.7 Closed Circuit Diving

Preparation

NOTICE

To use the SYMBIOS HUD for closed-circuit diving, first set the SYMBIOS HUD to closed-circuit mode in menu → DIVE SETTINGS → DIVE MODE → CCR.

Next, pair the SYMBIOS HUD with a wireless SYMBIOS CM eCCR interface. Various interfaces are available.

Set the diluent gas in menu → SETTINGS → GAS TABLE → DIL 1-3

Pair a tank pressure transmitter if you wish to have a tank pressure readout of the diluent tank.

O₂ Sensor Calibration

CCR O₂ sensors must be calibrated before diving.

Please consult your SYMBIOS CM eCCR user manual for specific instructions regarding O₂ sensor calibration.

Diving



This is a typical example of the main screen during a CCR dive with air as diluent (NX21). The HUD indicates the pO₂ of all the sensors, the current diving mode (CC), and the diluent used. The right bar graph indicates the tank pressure of the O₂ tank (98 bar). The left bar graph indicates the diluent pressure.



If the no-decompression limit is exceeded, the HUD indicates the decompression stop depth (in this example, 3 meters) and the estimated time to surface (5 minutes in CC mode).



If a pO₂ sensor reads a value above 1.6 bar/ATA, the value will blink white and red.



If a pO_2 sensor reads a value below 0.3 bar/ATA pO_2 , the value will blink red and blue.



If a pO_2 sensor is showing incorrect values, it can be excluded from the deco calculations. Sensors can be enabled/disabled from deco calculations in menu → SETTINGS → CCR SETTINGS → PO_2 SENSORS.

Bailout

If a pO_2 sensor displays values that are too low or too high, take immediate action—for example, bail out.

There are multiple ways to switch the SYMBIOS HUD to bailout mode:


— Menu → CCR BAILOUT

— In certain rebreathers, the SYMBIOS HUD is automatically switched to BAILOUT mode when the rebreather is equipped with a BOV with a sensor: for instance, the SYMBIOS CM eCCR.

In this example, the SYMBIOS HUD is switched to BAILOUT which is indicated with BO at the bottom of the screen.



If the SYMBIOS HUD is set to BAILOUT mode, the computer will propose the best breathing gas (similar to open circuit diving mode).

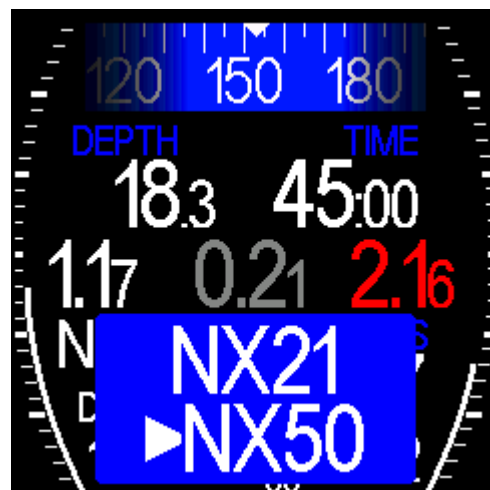

In this example, the current gas is set to NX21. The SYMBIOS HUD proposes that you switch to NX50.

After performing a gas switch, select the correct breathing gas. There are two possible ways to select the best gas:

- Select the proposed gas in menu → GAS TABLE.

- Long press button B to select the best gas. This, however, requires that the custom function for "Press and hold B button" is set to BEST GAS (menu → SYSTEM → CUSTOM FUNC → BEST GAS). For more advanced functions of the SYMBIOS HUD while diving with a SYMBIOS CM eCCR, please consult your SYMBIOS CM eCCR user manual.

NOTICE

After switching to bailout mode and the SYMBIOS HUD proposes a better breathing gas, select the best gas on the SYMBIOS HUD after performing the gas switch. There are two possible ways to select the best gas:

- Select the proposed gas in menu → GAS TABLE.

- Long press button B to select the best gas. This, however, requires that the custom function for "press and hold button B" is set to BEST GAS (menu → SYSTEM → CUSTOM FUNC → BEST GAS).

NOTICE

Some wireless transmitters will not start transmitting data until the pO_2 within the loop exceeds at least approximately 0.4–0.5 bar/ATA.

NOTICE

A CCR sensor calibration will only be successful when the analog sensors can output at least 38mV @ 1 bar/ATA pO_2 .

WARNING

If a pO_2 sensor is reading a pO_2 value below 0.3 bar/ATA, the value will blink white and blue. Take immediate action; for instance, bail out.

WARNING

If a pO_2 sensor is reading a pO_2 value above 1.6 bar/ATA, the value will blink white and red. Take immediate action; for instance, bail out.

WARNING

If the values are displayed in grey, this means that the SYMBIOS HUD is not receiving pO_2 data from a wireless transmitter. Read your backup display and act immediately.

WARNING

Do not dive with a rebreather without proper training and certification.

3.8 Closed Circuit Diving with Fixed Setpoint

The CCR FIX SP mode can be used for closed circuit diving with a fixed pO_2 setpoint. This is the preferred mode when the SYMBIOS HUD is not paired with a CCR. In this mode, you can pair the dive computer with tank transmitters for O_2 as well as diluent.

NOTICE

The setpoints can be selected in menu → CCR SETPOINT.

NOTICE

Switch between CCR and Bailout in menu → CCR Bailout.



This is an example of the screen during closed circuit diving with fixed setpoint. The left bar graph indicates the tank pressure of diluent (171 bar), and the right bar graph indicates the tank pressure of the O₂ tank (98 bar). Tank pod pressure transmitters are required to indicate the pressure of both oxygen and diluent gases.



If the no-decompression limit is exceeded, the computer indicates the decompression stop depth (in this example, 3 meters) and the estimated time to surface (5 minutes) in CC mode.

The closed-circuit time to surface estimate is based on the current pO₂ setting. Bailout time to surface estimation is based on the enabled gases in the gas table.




Example of a screen during open circuit bailout

Long press button B to cycle between CC and BO mode, Low Setpoint, and High Setpoint.

3.9 Bottom Timer

To use the SYMBIOS HUD as a bottom timer, first set the SYMBIOS HUD to bottom timer mode in menu → SETTINGS → BOTTOM TIMER.

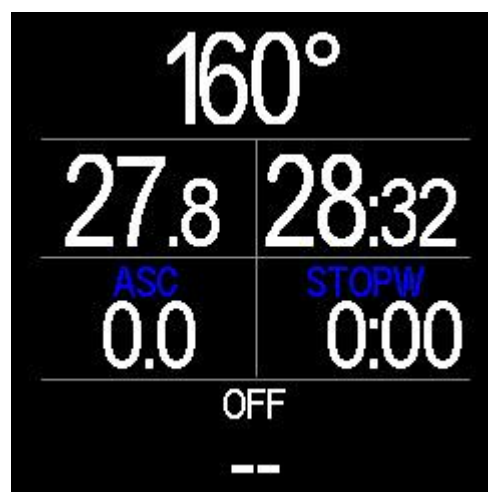


This is an example of the bottom timer screen. The top field indicates the compass heading. The second row indicates depth and dive time.

The right field in the third row shows the stopwatch.

The left field in the second row can be toggled between different values.

- Short press button B to toggle the lower left field between:
 - Current time and date
 - CNS% (when a tank pod is paired to a gas in the gas table)
 - pO_2 (when a tank pod is paired to a gas in the gas table)
 - Maximum depth
 - Average depth
 - Tank pressure of a transmitter paired to gas in the gas table
 - Ascent rate indicator
 - Battery level
- Long press the lower button to start/reset the stopwatch

A heading can be selected in menu → HEADING. If you select a heading, arrows next to the heading indicate toward the selected heading.

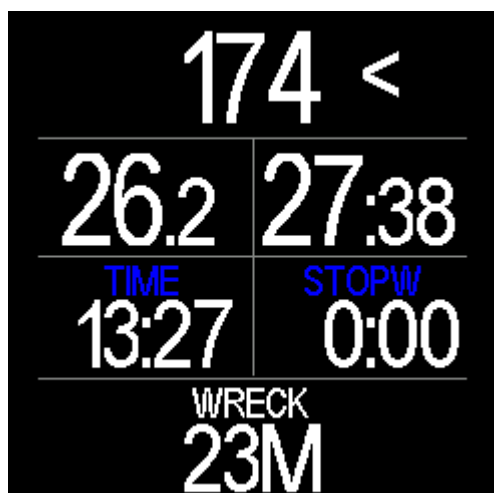

⚠ WARNING

In bottom timer mode, the SYMBIOS HUD does not perform decompression calculations.

3.10 Sidemount Diving

The sidemount diving mode is used for diving with more than one sidemount tank. For sidemount diving with just one tank, open circuit diving mode is the preferred mode.

The left tank is the first gas entry in the gas table. The right tank is the second gas entry in the gas table.

The left tank transmitter must be paired with the first entry in the gas table. The right tank transmitter needs to be paired with the second entry in the gas table.



This sample screen shows a depth of 24 meters and 18 minutes of dive time. The remaining no-decompression limit is 5 minutes. In this example, the remaining tank pressure of the left tank is 137 bar, and the remaining tank pressure of the right tank is 123 bar. Both pressure values are

also displayed via the left and right bar graph.



This sample screen shows a depth of 36.7 meters and 23 minutes of dive time. The current time to surface is 7 minutes, and the next deco stop is at 6 meters.



If the difference of the tank pressure between the two sidemount tanks is greater than 30 bar, you will be notified with a popup window.

NOTICE

A popup message will notify you of a pressure difference greater than 30 bar between the two sidemount tanks.

This function is only available, however, when the fraction of the two gases is the same and no decompression gas is carried.

3.11 Navigation

You can select and/or edit a target heading in menu → HEADING. You can set a compass declination in menu → SYSTEM → COMP DECLINATION.



In this example, the selected target heading is 127° and the current heading is 120°. A right-pointing arrow indicates that the target heading is right from the current heading.



Two arrows indicate that the current heading is equal to the target heading.



On this screen, the compass is represented with a moving scale. The 127° target heading is marked with a yellow line. The current heading is marked with a small triangle.

NOTICE


Before diving, make sure that the compass is correctly calibrated. See chapter 3.5 for compass calibration instructions.

3.12 Alarms and Notifications

The SYMBIOS HUD highlights potentially dangerous parameters using blinking colors. Additionally, pop up messages notify you of dangerous situations.



Tank pressure is too low: In this example, the tank pressure is 45 bar and blinking red and white.

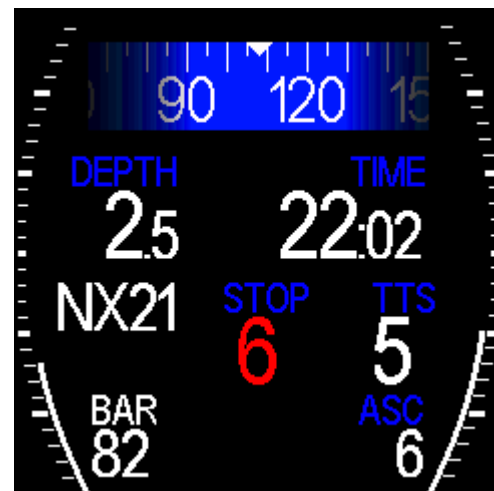

Decompression stop depth or ceiling violation: The decompression stop depth value will blink white and red. A pop up

warning will be visible if you violate the ceiling depth.



Gas MOD exceeded: If the selected pO_2 for the gas is exceeded, the depth value will blink white and red.



Safety stop incomplete: If the safety stop is not completed, a yellow warning will be visible at the end of the dive when the computer enters surface mode.



Tissues saturation reset: If the user performs a tissue saturation reset, a warning will appear while on the surface.



Battery low: When the battery level of the HUD is below 15%, a battery low warning alert will appear.

Notifications in Sidemount Mode



SWITCH SIDE will appear as a pop up if the tank pressure between left and right tank differs by more than 30 bar.

NOTICE

This function is only available if both the left and right tanks are equipped with tank pods paired to the SYMBIOS HUD.

Alarms in CCR mode




In CCR mode, if one sensor pO₂ level is below 0.3 bar/ATA, the pO₂ value of a sensor will blink red and blue.



In CCR mode, if one or more sensors pO₂ levels are above 1.6 bar/ATA, the pO₂ value of the sensor will blink white and red.



In CCR mode, if the average pO₂ value falls below 0.3 bar/ATA, the PO2 LOW warning will pop up.

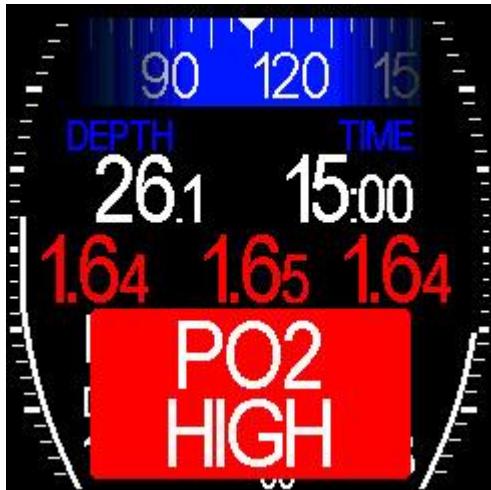

In CCR mode, if the average pO_2 value rises above 1.6 bar/ATA, the PO2 HIGH warning will pop up.



CCR BAT will pop up when the remaining battery capacity of the CCR is less than 20%.



NO CCR SIGNAL will pop up when the SYMBIOS HUD does not receive wireless data for more than 30 seconds.



CHECK SENS will pop up when the controller and sentinel read pO_2 values that differ by more than 0.1 bar/ATA.



SCRUB LOW will pop up when the scrubber timer is used and the remaining scrubber time is less than 15%.

For more advanced notifications while diving with a SYMBIOS CM eCCR, please consult the SYMBIOS CM eCCR user manual.

NOTICE

Press and hold both buttons to confirm an alarm and deactivate a pop up message or vibration alarm.

4 Specifications

4.1 General Specifications

- Maximum operational depth: 120 m/394 ft
- Full color transfective sunlight readable TFT Screen, 320 x 240 pixel, RGB
- Digital Pressure Sensor, 300 m/984 ft rated
- Depth resolution: 0.1 m/0.3 ft
- Temperature resolution 0.1 °C/32 °F
- Digital compass, tilt compensated
- 2 channel magnetic wireless interface, 125 kHz

- BT interface
- USB interface
- Housing made from glass fiber reinforced polyamide

- The depth of equipment certification according to EN250:2014 is 50 m.
- The air supply for equipment compliant with EN250:2014 shall meet the requirements for breathable air in accordance with EN 12021.

4.2 Decompression Algorithm

- Bühlmann ZH-L16C decompression model
- 16 compartments for nitrogen, 16 compartments for helium
- Gradient factors
- No-fly time indicator
- Automatic altitude adaption

AIR / NITROX / TRIMIX open circuit diving:

- 5 gas settings for open circuit diving

Closed circuit rebreather diving:

- 3 diluent gas setting for closed circuit diving

4.3 Electrical specifications

- 32 bit microprocessor
- Rechargeable Li Ion battery, 4.2 V, 300 mAh
- Rechargeable via USB, maximum charge current 350mA
- Autonomy in standby mode: 1 year

- 25 hours (display brightness set to 5) operation during diving
- Charge time 4 hours
- Interface: Wireless, Electromagnetic

4.4 Dive data storage

- 32 GB storage capacity
- Dive data storage interval in dive mode: 5 seconds
- Memory accessible via USB (SYMBIOS HUD is recognized as Mass Storage Device)
- Memory also accessible via wireless BT5.0 interface

4.5 Testing and validation

The SYMBIOS HUD was tested according to various EU-Normatives and has passed those tests, thus is CE compliant. For more information, please see section CE and FCC.

In addition to many test dives in sea and fresh water, numerous simulated dives were carried out in the laboratory and in a hyperbaric chamber to validate the correct function of the computer and the correct implementation of the decompression model. The code was validated against Eric C Baker's implementation of the Bühlmann ZH-L16 algorithm with Gradient Factor extension.

The SYMBIOS HUD together with the SYMBIOS Tank Pod were tested according to EN250:2014.

Prior to shipment, your SYMBIOS HUD was tested for water and pressure resistance.

5 Troubleshooting

The SYMBIOS HUD does not switch on.

- Charge the SYMBIOS HUD for at least 3 hours. If the SYMBIOS HUD is completely discharged, it loses all decompression information and is reset to default settings. It should restart shortly after charging begins.

The SYMBIOS HUD is connected to a USB charger but does not charge.

- Check the cable and the connector pins for corrosion and dirt. Clean if possible.
- Use a charger that can output at least 800mA and a voltage of 5V.

The SYMBIOS HUD is outside the water, but it is in dive mode and the displayed depth is greater than 0.5 m/1 ft.

- This can happen when the SYMBIOS HUD is exposed to a sudden drop of atmospheric pressure. In this case, you must reset the SYMBIOS HUD. Simply attach the USB cable to the SYMBIOS HUD and plug it into a charger. In this specific case, the SYMBIOS HUD will be reset after a few seconds. All decompression information and user settings are lost after a reset.

The tilt angle is incorrect.

- Check if the tilt sensor is paired.
- Perform a calibration of the tilt sensor.

The tank pressure is not reported correctly.

- Check if the SYMBIOS Tank Pod is paired correctly.
- Check the battery voltage of the SYMBIOS Tank Pod in the pairing menu.
- Check if the SYMBIOS Tank Pod is pressurized.

– Check if the SYMBIOS Tank Pod is within the maximum transmission range of 90 cm/35 in.

6 Firmware Update

Complete the following steps to perform a firmware update:

1. Connect the SYMBIOS HUD to your PC.
2. The SYMBIOS HUD will be recognized as a mass storage device.
3. Download the latest firmware.
4. Unpack the firmware zip file: RNO_HUD_FW_Vx_xx_xx.zip.
5. Copy the files from the zip file to the mass storage device.
6. Safely remove the mass storage device.
7. Disconnect the SYMBIOS HUD from your PC.

The SYMBIOS HUD will then update with the new firmware.

Firmware updates can also be performed using the HALCYON Dive App.

NOTICE

The version of the firmware on your SYMBIOS HUD is shown in menu → SYSTEM → FIRMWARE VERSION.

NOTICE

Make sure that the SYMBIOS HUD is fully charged before performing a firmware update.

! WARNING

All decompression information and settings may be lost after a firmware update.

! WARNING

Avoid a firmware update between repetitive diving. Performing a firmware update between dives will cause the SYMBIOS HUD to lose decompression data and the remaining compartment inert gas data from the previous dives; thus, the no-decompression times and decompression calculations for the next dives may be incorrect.

7 Warranty

HALCYON LIMITED WARRANTY

HALCYON warrants that, during the warranty period, HALCYON or a HALCYON authorized service center will, at its sole discretion, remedy defects in materials or workmanship free of charge either by repairing, replacing, or refunding subject to the terms and conditions of this limited warranty.

Warranty period(s):

- Begins at the date of original purchase.
- Includes two years for products unless otherwise specified.
- Includes one year for accessories.
- Includes six months for rechargeable batteries.

The limited warranty does not cover:

- Normal wear and tear such as scratches, abrasions, alteration of the color, or defects caused by rough handling
- Defects or damage resulting from use contrary to intended or recommended use, improper care, negligence, and/or accidents such as dropping or crushing

– Printed materials and packaging

The limited period is not enforceable if the product or accessory has been:

- Opened
- Repaired using unauthorized spare parts
- Repaired by an unauthorized service center
- Exposed to chemicals including, but not limited to, sunscreen sprays, lotions, creams, and insect repellents

7.1 Limitations of Liability

WITH THE PURCHASE OF THE SYMBIOS HUD, YOU HEREBY AGREE TO THE FOLLOWING EXCLUSIONS AND LIMITATIONS OF HALCYON'S LIABILITY TO YOU.

YOU AGREE AND UNDERSTAND THAT SCUBA DIVING IS A HIGH RISK, POSSIBLY LIFE-THREATENING ACTIVITY, AND THE USE OF THE SYMBIOS HUD IS IN NO WAY A SUBSTITUTE FOR PROPER SCUBA TRAINING AND VALID CERTIFICATION.

BECAUSE OF THE NUMBER OF VARIABLE SCENARIOS, AS WELL AS THE DIFFERENT DEGREES TO WHICH THEY MAY AFFECT INDIVIDUALS ENGAGED IN SCUBA DIVING, YOU UNDERSTAND AND AGREE THAT THE USE OF THIS PRODUCT WILL NOT PREVENT DECOMPRESSION SICKNESS (DCS) OR ANY OTHER CONDITION OR INJURY INCURRED WHILE USING THIS PRODUCT. HALCYON DOES NOT WARRANT NOR DOES IT GUARANTEE THAT USE OF THIS PRODUCT WILL PREVENT DECOMPRESSION SICKNESS OR ANY OTHER CONDITION OR INJURY INCURRED WHILE USING THIS PRODUCT.

THESE INFLUENCING VARIABLES MAY INCLUDE, BUT ARE NOT LIMITED TO, DEHYDRATION, OBESITY, ADVANCED AGE, PHYSICAL INJURIES, OR OTHER PHYSICAL OR MENTAL CONDITIONS OF THE DIVER, AS WELL AS ENVIRONMENTAL EXTREMES OF HEAT OR COLD, POOR TRAINING, OR UNSOUND DIVING PRACTICES, ANY OF WHICH MAY PROMOTE THE ONSET OF DECOMPRESSION SICKNESS OR CAUSE OTHER HARMFUL EFFECTS.

THE SYMBIOS HUD WAS TESTED ACCORDING TO EN13319 AND WAS EVALUATED IN NUMEROUS TEST DIVES. HOWEVER, THERE MAY STILL BE ERRORS IN THE SOFTWARE, THAT WERE NOT IDENTIFIED YET AND THAT MAY LEAD TO MALFUNCTIONS OF THE SYMBIOS HUD. THEREFORE, HALCYON RECOMMENDS THAT YOU ALWAYS CARRY AND USE A BACKUP DIVE COMPUTER OR A DIVE TABLE IN COMBINATION WITH A DEPTH GAUGE AND A WATCH.

YOU AGREE THAT YOU UNDERSTAND AND ACCEPT ALL RISKS ASSOCIATED WITH DIVING, AND THAT HALCYON, ITS ELECTED AND APPOINTED OFFICIALS, EMPLOYEES, VOLUNTEERS, OR OTHERS WORKING ON BEHALF OF HALCYON ARE NOT LIABLE TO YOU OR ANY OTHER PERSON, INCLUDING YOUR HEIRS, EXECUTORS OR PERSONAL REPRESENTATIVES, FOR ANY LOSS, DAMAGE, COST, EXPENSE OR CLAIM ARISING FROM, CAUSED BY, OR RELATING TO YOUR PERSONAL INJURY OR DEATH WHILE DIVING, EVEN IF YOUR PERSONAL INJURY OR DEATH IS CAUSED, IN WHOLE OR IN PART, AND DIRECTLY OR INDIRECTLY, BY THE PURCHASE OF THE SYMBIOS HUD OR YOUR USE THEREOF, OR ARISING FROM BREACH OF THE WARRANTY, BREACH OF CONTRACT,

NEGLIGENCE, STRICT TORT, OR ANY OTHER LEGAL OR EQUITABLE THEORY, EVEN IF HALCYON KNEW, OR SHOULD HAVE KNOWN OF THE LIKELIHOOD OF SUCH DAMAGES, AND REGARDLESS OF WHETHER OR NOT THE HEAD UP DIVING COMPUTER FUNCTIONED PROPERLY OR WAS DEFECTIVE IN ANY WAY. HALCYON SHALL NOT BE LIABLE FOR DELAY IN RENDERING SERVICE UNDER THE LIMITED WARRANTY, OR LOSS OF USE DURING THE TIME THE PRODUCT IS BEING REPAIRED.

YOU HEREBY IRREVOCABLY WAIVE AND RELEASE HALCYON, ITS ELECTED AND APPOINTED OFFICIALS, EMPLOYEES, VOLUNTEERS, OR OTHERS WORKING ON BEHALF OF HALCYON FROM ANY LIABILITY OR OBLIGATION TO YOU OR YOUR HEIRS, EXECUTORS OR PERSONAL REPRESENTATIVES FOR ANY LOSS, DAMAGE, COST, EXPENSE, OR CLAIM ARISING OUT OF, CAUSED BY OR RELATING TO YOUR PERSONAL INJURY OR DEATH WHILE DIVING, EVEN IF YOUR PERSONAL INJURY OR DEATH IS CAUSED, IN WHOLE OR IN PART AND DIRECTLY OR INDIRECTLY, BY THE SYMBIOS HUD OR YOUR USE OF THE SYMBIOS HUD, OR ARISING FROM BREACH OF THE WARRANTY, BREACH OF CONTRACT, NEGLIGENCE, STRICT TORT, OR ANY OTHER LEGAL OR EQUITABLE THEORY, EVEN IF HALCYON KNEW, OR SHOULD HAVE KNOWN OF THE LIKELIHOOD OF SUCH DAMAGES, AND REGARDLESS OF WHETHER OR NOT THE SYMBIOS HUD FUNCTIONED PROPERLY OR WAS DEFECTIVE IN ANY WAY.

YOU MUST READ AND ACCEPT THE AGREEMENT FOR ALL LIMITATIONS AND EXCLUSIONS OF HALCYON'S LIABILITY TO YOU.

8 CE

The SYMBIOS HUD is in conformity with:

- EN250:2014: The combination of a Halcyon SYMBIOS HUD and the Halcyon Symbios Tank Pod is a personal protective equipment under the Regulation (EU) 2016/425. SGS Fimko Oy, Takomotie 8, 00380 Helsinki, Notified Body No: 0598, performed EU type-examination (Module B) of the Regulation (EU) 2016/425 Personal Protective Equipment and issued EU type-examination certificate Nr 0598/PPE/24/5116. The EC Type examination of the SYMBIOS HUD together with the Halcyon Symbios Tank Pod was conducted by SGS Fimko Oy, Notified Body No. 0598. In this case, the SYMBIOS HUD is in conformity with EN250:2014 – respiratory equipment – opencircuit self-contained compressed air diving apparatus – requirements, testing and marking – clause 6.11.1 Pressure Indicator for use with equipment that is compliant with EN12021. The air supply for equipment compliant with EN250:2014 shall meet the requirements for breathable air in accordance with EN 12021. The depth of equipment certification is 50 m. The Halcyon Symbios Handset or Symbios HUD in combination with the Halcyon Symbios Tank Pod are subject to the conformity assessment procedure conformity to type based on the quality assurance of the production process plus supervised product checks at random intervals (Module C2) under surveillance of the Notified Body SGS Fimko Oy, Helsinki; Notified Body 0598.
- EN13319 (European standard for depth gauges)
- Regulation (EU) 2014/53, Radio Equipment Directive
- EN 300 330:2017 V2.1.1 (Radio spectrum), Short Range Devices (SRD); Radio

equipment in the frequency range 9 kHz to 25 MHz and inductive loop systems in the frequency range 9 kHz to 30 MHz; Harmonised Standard covering the essential requirements of article 3.2 of Directive 2014/53/EU.

– EN 55032:2015 + A1:2020 + A11:2020 (EMC), Electromagnetic compatibility of multimedia equipment – Emission requirements

The full text of the EU declaration of conformity is available at the following internet address:

https://halcyon.net/files/ce-declarations/CE_Decl_HUD.pdf

9 Identification

The SYMBIOS HUD is laser marked with a label containing information about the manufacturer, the model, CE and FCC symbols, and the serial number indicating manufacturing year and month. The first 2 digits of the serial number are the last 2 digits of the production year.



9.1 FCC

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/ TV technician for help.

10 Info

Halcyon Dive Systems
24587 NW 178th Place
High Springs, FL 32643
USA

info@halcyon.net

Tel: +1.800.HALCYON (425.2966)

European point of contact:
Halcyon Europe Sp z o.o.
Wodnika 50, Pav 6
80-299 Gdańsk
Poland

HALCYON™ 